



MicroLWCC

Low volume flow cell for FIA, HPLC and Process Analysis



MicroLWCC (WPI #**LWCC-M-10**, **LWCC-M-50**, **LWCC-M-100**) is a new fiber optic low volume flow cell for UV/VIS/NIR absorbance analysis. The LWCC-M-10 has a 10mm pathlength, the LWCC-M-50 has a 50mm pathlength and the LWCC-M-100 has a 100mm pathlength. Based on WPI's established liquid core waveguide technology, the analyte solution functions as the core of a fluid filled light waveguide. Wetted parts in the sample cell light path are PEEK, fused silica and Teflon. Optical fibers are used to transport light to and from the sample cell. The cell can be used in biochemistry for DNA, RNA & protein quantification, colorimetric nutrient and trace metal analysis, drug discovery and dissolution testing, process control, and HPLC analysis.

SPECIFICATIONS

	M-10	M-50	M-100
Optical Pathlength	10mm	50mm	100mm
Internal Volume	2.4µL	12µL	24µL
Wavelength Range	200 – 1000nm		
Fiber Connection (SMA)		500µm	
Transmission @ 254 nm *	> 40%	> 30%	> 10%
Transmission @ 540nm *	> 50%	> 40%	> 20%
Maximum Pressure		1000 PSI	
Refractive Index @ 280 nm**	< 7 mAU	< 15mAU	
Wetted Material	PEEK, Fused Silica, PTFE		

* Reference: Two 600 µm fibers, butt-coupled

** Measured using ASTM E 685 - 93, includes intrinsic solvent absorbance

WPI U.S. Patents: 5,444,807; 5,570,447; 5,604,587; 6,603,556; 6,385,380.



MicroLWCC

Low volume flow cell for FIA, HPLC and Process Analysis

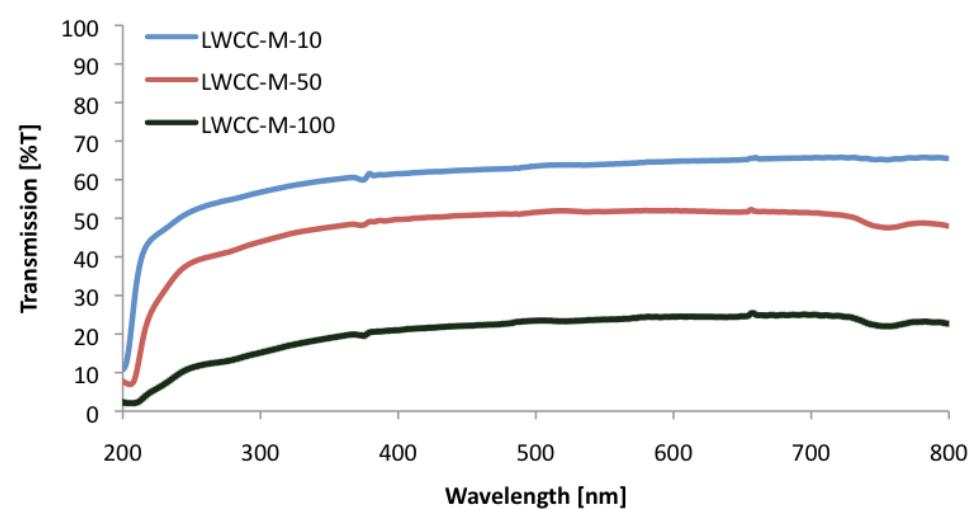


Fig.1—This graph show the percentage of light transmission at various wavelengths. The higher the light transmission percentage, the greater the resolution.

References

- M. Belz, "Simple and sensitive protein detection system using UV LEDs and liquid core waveguides", Advanced Environmental, Chemical, and Biological Sensing Technologies V, Optics East, Oct 2007, Proc. SPIE, Vol. 6755, 675505
- M. Belz, F. A. Klein, H. S. Eckhardt, K. Klein, D. Dinges, K. T. V. Grattan, "Optical Detection Techniques and Light Delivery with UV LEDs and Optical Fibres", Third

International Conference on Optical and Laser Diagnostics, Proc. IOP, City University, London, UK, May 2007.

M. Belz, P. Dress, A. Sukhitskiy, S. Liu, "Linearity and effective optical pathlength of liquid waveguide capillary cells", Part of the SPIE Conference on Internal Standardization and Calibration; Architectures for Chemical Sensors, Boston Massachusetts, September 1999, SPIE Vol. 3856, 271-281.

World Precision Instruments, Inc.

USA: International Trade Center, 175 Sarasota Center Boulevard, Sarasota FL 34240-9258 USA

Tel: 941-371-1003 • **Fax:** 941-377-5428 • **E-mail:** info@wpiinc.com • **Internet:** <http://www.wpiinc.com>

Germany: Zossener Str. 55, 10961 Berlin, Germany • Tel: 030-6188845 • Fax: 030-6188670 • E-mail: wpide@wpi-europe.com

China & Hong Kong: WPI Shanghai Trading Co., Ltd. • Tel: +86 688 85517 • E-mail: ChinaSales@china.wpiinc.com

UK: Astonbury Farm Business Centre • Aston, Stevenage, Hertfordshire SG2 7EG England • Tel: 01438-880025 • E-mail: wpiuk@wpi-europe.com